



## HDMD PRO DICOM Conformance Statement

**Med X Change, Inc.**

**HDMD PRO**

**DICOM Conformance Statement**

# HDMD PRO DICOM Conformance Statement

## Contents

- 1 Overview ..... 3
- 2 Introduction ..... 3
  - 2.1 General information ..... 3
  - 2.2 Scope ..... 3
  - 2.3 Audience ..... 3
  - 2.4 How to Use This Document ..... 3
  - 2.5 Warning Regarding Connectivity ..... 5
- 3 Definitions, Terms and Abbreviations ..... 5
  - 3.1 References ..... 6
- 4 Networking ..... 7
  - 4.1 Implementation Model ..... 7
    - 4.1.1 Application Data Flow ..... 7
    - 4.1.2 Functional Definition of AE's ..... 8
    - 4.1.3 Sequencing of Real Work Activities ..... 8
  - 4.2 AE Specifications ..... 9
    - 4.2.1 Workflow AE Specifications ..... 9
    - 4.2.2 Storage AE Specifications ..... 16
  - 4.3 Network Interfaces ..... 21
  - 4.4 Configuration ..... 21
- 5 Media Interchange ..... 22
- 6 Support of Character Sets ..... 22
- 7 Security ..... 22
  - 7.1 Security Profiles ..... 22
  - 7.2 Application Level Security ..... 22
- 8 Annexures ..... 23
  - 8.1 IOD Contents ..... 23
    - 8.1.1 Secondary Capture IOD ..... 23
    - 8.1.2 Multi-frame True Color Secondary Capture IOD ..... 25
  - 8.2 Attribute Mapping ..... **Error! Bookmark not defined.**

**HDMD PRO DICOM Conformance Statement**

**1 Overview**

This document provides the details of the DICOM conformance statement for the Med X Change HDMD PRO. This document is structured as suggested in the DICOM Standard (PS 3.2, 2011).

*Table 1-1 – Network Services*

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
<b>Transfer</b>		
Secondary Capture Image Storage	Yes	No
Multi-frame Secondary Capture Image Storage	Yes	No
<b>Workflow</b>		
Modality Worklist Information Model – FIND	Yes	No
<b>Other</b>		
Verification	Yes	No

**2 Introduction**

**2.1 General information**

This document specifies the DICOM conformance statement of the Med X Change HDMD PRO providing acquisition, study documentation, and archive capabilities.

**2.2 Scope**

This document applies to Med X Change HDMD PRO xxxx (and higher).

**2.3 Audience**

This document is intended for hospital staff, health system integrators, software designers, and implementers of the Med X Change HDMD PRO. It is assumed that the reader has a working understanding of DICOM.

**2.4 How to Use This Document**

This statement consists of 5 important features that one should compare with other devices to determine connectivity:

- 1. Implementation model:** The Implementation model describes the functional relationship between the device, the so-called “real-world activities” which initiate a certain DICOM functionality, and the DICOM services. A DICOM service is implemented on a device by a software process, which is called an “Application Entity” (AE). Each AE has a unique name called the AE Title, which is used to identify it to other AE’s. The AE Title is configurable to avoid two devices with the same name on a network. The “bubble diagram” (Application Data Flow Diagram) shows the interaction of the AE with the outside world across the dashed line, i.e. the DICOM interface. The “sequencing of real

## HDMD PRO DICOM Conformance Statement

world activities” describes the interaction using a time-scale, i.e. showing the sequence of events.

2. **AE Specifications:** Each AE supports one or more Service-Object-Pair (SOP) classes, which define the basic functionality. A SOP class consists of a combination of an Object or Information model with specific DICOM services. An example of such a SOP class is the VL Image Storage class, which consists of the combination of the DICOM C\_STORE command with the VL Image object. Each of these classes is uniquely identified by a unique identification number (UID), which is issued by the NEMA. In addition, the “role” of the AE is specified, i.e. User or Provider, which can be compared with acting as a Client or Server. In DICOM terms, this is called a Service Class User (SCU) or Service Class Provider (SCP). To interconnect with another device, the SOP classes as well as their role (SCU or SCP) have to be matched, i.e. a SCU has to match a SCP at another device with an identical SOP class. Make sure to compare the SOP Class UID itself, not the description because there are SOP classes which have the same name, but support a different (newer) Object, which is identified by a different SOP Class UID.
3. **Presentation Context:** Each SOP class supports a particular presentation context, which is the combination of the SOP class as specified in AE Specifications and the Transfer Syntax. The Transfer Syntax defines the encoding of the DICOM basic elements, i.e. its attributes and how the data is represented e.g. with a data type definition. The encoding of the data type as part of the message, or value representation (VR), can be done in two ways - implicitly or explicitly. If a device supports explicit VR transfer syntax, it means that the transmitted data will include the VR information along with data and attribute tags. Implicit VR means that the VR information will not be included, and the receiving application must determine the VR type from the Attribute tag. For example, when receiving the Attribute “Patient Name” in explicit transfer syntax, there is an additional “Person Name” (“PN”) field to identify the Value Representation. In the case of an implicit VR, this is assumed to be known by the receiver and not explicitly specified that this field has a type of “Person Name”. Lastly, compression can be applied, such as JPEG, which is specified in the transfer syntax. The Transfer syntax of two devices has to match in order for them to communicate.
4. **Communication Profiles:** This section specifies the communication options. In practice, each device always supports application level interface to the OSI level 4 (Transport layer), i.e. TCP/IP stack. However, the physical media of two devices have to match for connectivity. Note that matching physical media can be achieved by standard off the shelf devices. For example, if one device supports standard Ethernet 100BaseT, it can be bridged to a Gigabit Ethernet, or whatever is supported.
5. **Supported Attributes:** Many devices specify which DICOM attributes they require and/or store in their internal database. It is important to compare these against the source of the information, particularly if a device requires certain attributes to accomplish specific functionality such as 3-D viewing, image processing, etc. A mismatch could have the effect that certain functionality or applications might fail.

## HDMD PRO DICOM Conformance Statement

---

### 2.5 Warning Regarding Connectivity

The DICOM conformance statement provides a knowledgeable user with the information required in determining whether and to what extent independent DICOM implementations may be able to interoperate. However, the information contained in a DICOM conformance statement is not sufficient to ensure independent implementations will, in fact, be able to interoperate.

The user or system integrator must be aware of the following potential issues related to interoperability:

- Using only the information provided by this conformance statement does not guarantee interoperability of Med X Change equipment with non-Med X Change equipment. It is the user's (or system integrator's) responsibility to analyze thoroughly the application requirements and objectives to determine if they can be met by the connection of Med X Change equipment to non-Med X Change equipment.
- Med X Change equipment has been tested to assure that the actual implementation of the DICOM interface corresponds with this conformance statement. It is the responsibility of the user (or system integrator) to specify and carry out additional validation testing, which covers a broad spectrum of potential interactions between the independent implementations.
- Med X Change reserves the right to make changes to its products or to discontinue their delivery. Therefore, the user (or system integrator) should ensure that any future versions of Med X Change or non-Med X Change equipment are regression tested to verify that new software releases have not adversely impacted the ability to interoperate.

Med X Change provides this documentation "as is" without warranty of any kind, either expressed or implied, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose. Some states or countries do not allow disclaimers of express or implied warranties in certain transactions; therefore, this statement may not apply to you.

No part of this publication may be reproduced, transmitted, transcribed, recorded, or translated into any language in any form or by any means, electronic, magnetic, optical, chemical, physical, or otherwise without the express written permission of an authorized officer of Med X Change.

Med X Change reserves the right to correct this publication and to make changes to its contents without the obligation of informing anyone of these revisions or changes.

### 3 Definitions, Terms and Abbreviations

Definitions, terms, and abbreviations used in this document are defined within the different parts of the DICOM standard. Abbreviations and terms are as follows:

AE DICOM Application Entity

AET Application Entity Title

- ELE Explicit Little Endian
- ILE Implicit Little Endian
- EBE Explicit Big Endian
- IBE Implicit Big Endian
- IOD (DICOM) Information Object Definition
- IM Information Model
- ISO International Organization for Standardization
- O Optional Key Attribute
- PDU DICOM Protocol Data Unit
- R Required Key Attribute
- SC Secondary Capture
- SCP DICOM Service Class Provider (DICOM server)
- SCU DICOM Service Class User (DICOM client)
- SOP DICOM Service-Object Pair
- U Unique Key Attribute
- VL Visible Light

### **3.1 References**


[DICOM] Digital Imaging and Communications in Medicine (DICOM), NEMA PS 3.1-3.18, 2011

# HDMD PRO DICOM Conformance Statement

## 4 Networking

### 4.1 Implementation Model

#### 4.1.1 Application Data Flow

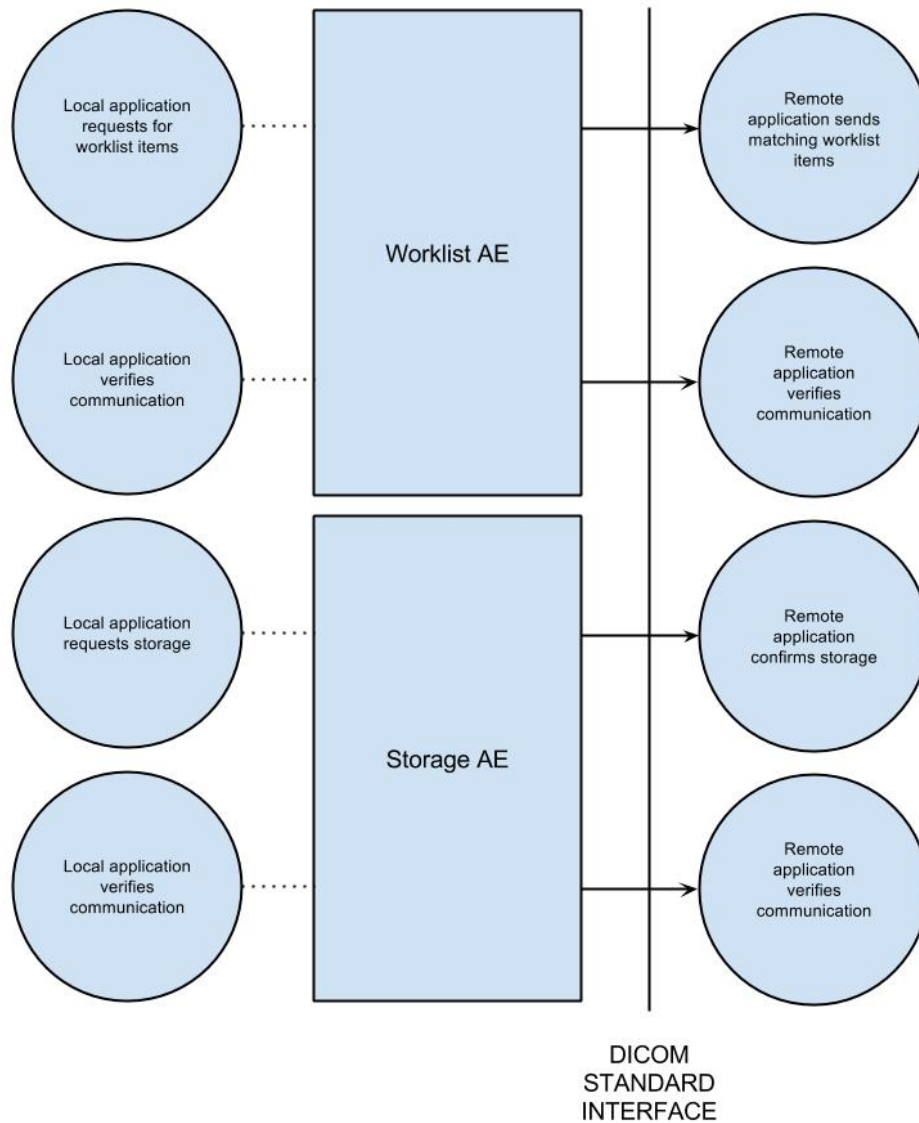

*Figure 1 Application Data Flow*

HDMD PRO exports images using DICOM Store Service. The following AE's describe the DICOM implementation of the HDMD PRO:

- The Worklist AE queries an external workflow management system for work items to be performed on the HDMD PRO.

## HDMD PRO DICOM Conformance Statement

- The Storage AE is responsible for storing the information created by the system (image) to other applications either automatically or upon operator commands.

### **4.1.2 Functional Definition of AE's**

#### **4.1.2.1 Worklist AE**

The Worklist AE acts as a SCU of the Basic Worklist Management Service Class. On user action, a query is performed to an external worklist manager and a set of worklist items matching the query is received. The received data is displayed on the user interface. A worklist item is selected for examination and all the data for that item along with the captures images is stored in the local database within the HDMD PRO.

#### **4.1.2.2 Storage AE**

The Storage AE is responsible for exporting the images from the HDMD PRO. Upon the Store, DICOM Instances are sent to the external application using DICOM Storage Service.

### **4.1.3 Sequencing of Real Work Activities**

A typical sequence is as follow:



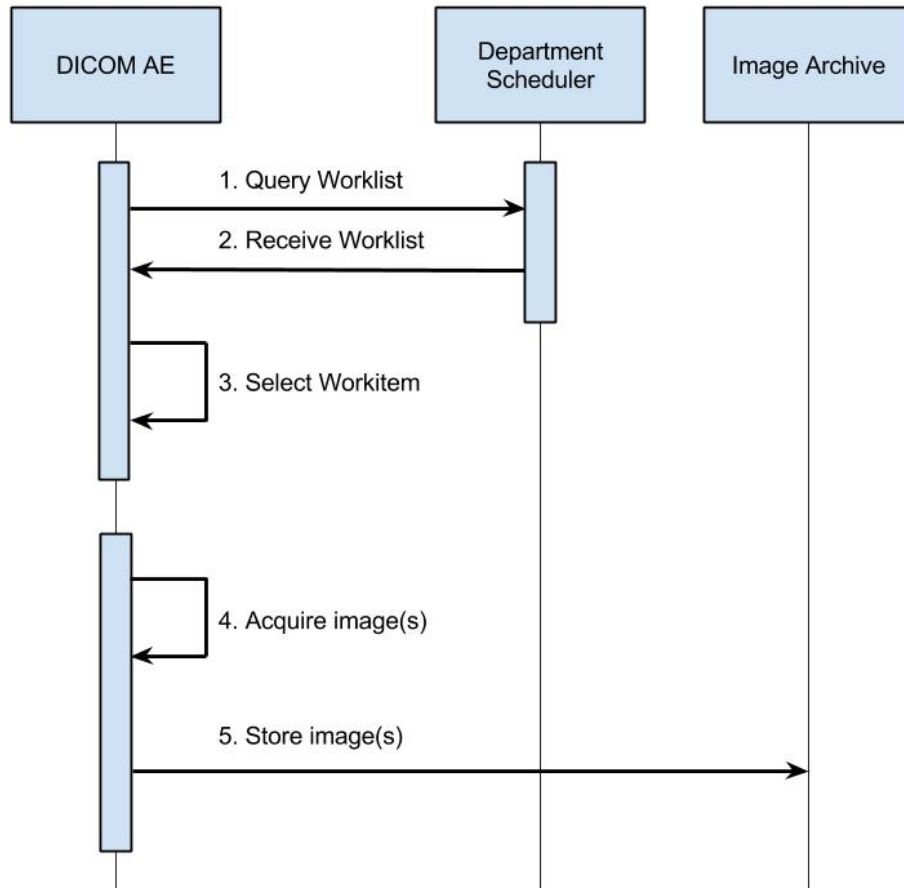


Figure 2 Sequence of Real World activities

1. A Worklist query can be initiated manually by a user or automatically.
2. The worklist is received. Patient demographics and order information is stored in the local database and displayed to the user upon request.
3. For unscheduled exams, the patient information will be entered manually; otherwise the work item (worklist entry) will be selected.
4. Still images and videos are acquired.
5. The acquired data is sent to a DICOM destination automatically or initiated by the user.

## 4.2 AE Specifications

### 4.2.1 Workflow AE Specifications

#### 4.2.1.1 SOP Classes

This AE provides standard conformance to the following SOP classes.

Table 4-1 – SOP Classes for Worklist AE

SOP Class Name	SOP Class UID	SCU	SCP
----------------	---------------	-----	-----

HDMD PRO DICOM Conformance Statement

Verification	1.2.840.10008.1.1	Yes	No
Modality Worklist Query	1.2.840.10008.5.1.4.31	Yes	No

**4.2.1.2 Association Policies**

**4.2.1.2.1 General**

The DICOM standard application context name for DICOM 3.0 is always proposed.

*Table 4-2 – General DICOM for Worklist AE*

Application Context Name	1.2.840.10008.3.1.1.1
Maximum PDU Size proposed	16384

**4.2.1.2.2 Number of Associations**

*Table 4-3 – Number of Associations as association initiator for Worklist AE*

Maximum number of simultaneous associations	1
---	---

The Workflow AE initiates association with an external AE in response to a user action in the application GUI.

**4.2.1.2.3 Asynchronous Nature**

The Workflow AE does not support multiple outstanding transactions.

**4.2.1.2.4 Implementation Identifying Information**

*Table 4-4 – DICOM Implementation Class and Version for STORAGE-SCP*

Implementation Class UID	1.2.276.0.7230010.3.0.9.9.1
Implementation Version Name	MED_X_CHANGE

**4.2.1.3 Association Initiation Policies**

**4.2.1.3.1 Activity – Verify Communications (SCU)**

**4.2.1.3.1.1 Description and Sequencing of Events**

The Worklist AE sends DICOM verification requests when the user requests a test of validity of a DICOM connection through the GUI.

**4.2.1.3.1.2 Proposed Presentation Contexts**

The HDMD PRO will propose Presentation Contexts as shown in the following table:

*Table 4-5 – Proposed Presentation Contexts for Activity Verify Communication*

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext Neg.
Name	UID	Name	UID		
Verification	1.2.840.10008	ELE	1.2.840.10008.1.2.1	SCU	None
		ILE	1.2.840.10008.1.2		

## HDMD PRO DICOM Conformance Statement

---

### **4.2.1.3.1.3 SOP Specific Conformance – Verification SOP Class**

The Storage AE provides standard conformance to the Verification SOP Class as an SCU. If the C-ECHO request was successfully received by external verification SCP, a 0000 (Success) status code will be returned in the C-ECHO response. Otherwise, a C000 (Error – Cannot Understand) status code will be returned in the C-ECHO response.


### **4.2.1.3.2 Activity- Query Worklist**

#### **4.2.1.3.2.1 Description and Sequence of Events**

The worklist query is initiated automatically when the user visits the worklist and can also be initiated manually with filters applied. A search dialog is present on the GUI for entering the data as search criteria. When the query is initiated on user request/automatically, the data from the dialog will be inserted as matching keys into the query. On initiation of a request, HDMD PRO will build an identifier for the C-FIND request; this will initiate an association to send the request and will wait for worklist responses. After retrieval of all responses, the application will access the internal worklist queue to display all the responses on the GUI and allow the user to select a specific patient/study for examination.

There is no mechanism to prevent system overflow. All worklist records retrieved will be displayed.

The HDMD PRO will initiate an association to issue a C-FIND request according to the Modality Worklist Information Model.

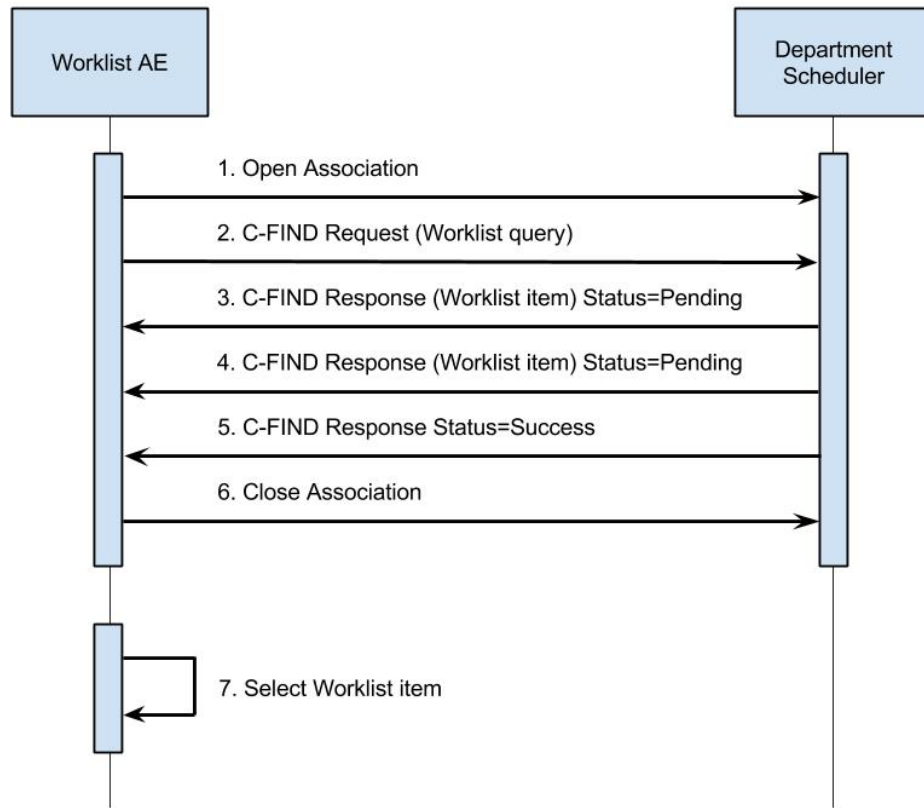

*Figure 3 Sequence of Events – Worklist query*

A possible sequence of interactions between the Worklist AE and the Departmental Scheduler (e.g. a device such as a RIS or HIS which supports the Modality Worklist SOP Class as an SCP) is illustrated in the figure above:

1. The Worklist AE opens an association with the Departmental Scheduler.
2. The Worklist AE sends a C-FIND request to the Departmental Scheduler containing the Worklist query attributes.
3. The Departmental Scheduler returns a C-FIND response containing the requested attributes of the first matching worklist item.
4. The Departmental Scheduler returns another C-FIND response contained the requested attributes of the second matching worklist item.
5. The Departmental Scheduler returns a final C-FIND response with Success status indicating that no further matching worklist items exist.
6. (This example assumes only 2 worklist items match the requested query).
7. The Worklist AE closes the association with the Departmental Scheduler.
8. The user selects a worklist item from the received responses and prepares to acquire new images for the selected item.

HDMD PRO DICOM Conformance Statement

**4.2.1.3.2.2 Proposed Presentation Contexts**

The HDMD PRO will propose Presentation Contexts as shown in the following table:

*Table 4-6 – Proposed Presentation Contexts for Activity Query Worklist*

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext Neg.
Name	UID	Name	UID		
Modality Worklist Information Model – FIND	1.2.840.10008.5.1.4.31	ELE	1.2.840.10008.1.2.1	SCU	None
		EBE	1.2.840.10008.1.2.2		
		ILE	1.2.840.10008.1.2		

**4.2.1.3.2.3 SOP Specific Conformance Statement for MWL SOP Class**

The attributes listed below are sent with the Modality Worklist Query.

In the following table, an S in the M (Matching) column means single value matching, W means wild card matching, and R means Range matching. An X in the Q (Query) column indicates a matching key that the user can interactively set. An X in the D (Display) column means that item is displayed in the HDMD PRO worklist, and an X in the IOD (Information Object Definition) column indicates the value that is returned in the response is used in the image instances created by the HDMD PRO for that procedure.

*Table 4-7 – Worklist Request Identifier*

Module Name Attribute Name	Tag	VR	M	Q	D	IOD
<b>Scheduled Procedure Step</b>						
Scheduled Procedure Step Sequence	(0040,0100)	SQ				
➤ Modality	(0008,0060)	CS	S	X	X	X
➤ Scheduled Procedure Step Start Date	(0040,0002)	DA	R	X	X	X
➤ Scheduled Station AE Title	(0040,0001)	AE	S	X		
➤ Scheduled Procedure Step Start Time	(0040,0003)	TM			X	X
➤ Scheduled Station Name	(0040,0010)	SH				X
<b>Requested Procedure</b>						
Study Instance UID	(0020,000D)	UI				X
Requested Procedure ID	(0040,1001)	SH			X	
Requested Procedure Description	(0032,1060)	LO			X	
<b>Image Service Request</b>						
Scheduled Performing Physician Name	(0040,0006)	PN			X	X
Accession Number	(0008,0050)	SH			X	X
Referring Physician Name	(0008,0090)	PN			X	X
<b>Patient Identification</b>						
Patient Name	(0010,0010)	PN			X	X

HDMD PRO DICOM Conformance Statement

Patient ID	(0010,0020)	LO	S	X	X	X
<b>Patient Demographic</b>						
Patient Birth Date	(0010,0030)	DA			X	X
Patient Sex	(0010,0040)	CS			X	X

The response behavior is described as below.

*Table 4-8 – MWL C-FIND Response Status Handling Behavior*

Service Status	Further Meaning	Error Code	Behavior
Success	Matching is complete	0000	The SCP has completed the matches. Worklist items are available for display or further processing.
Refused	Out of Resources	A700	The Association is released and the worklist query is marked as failed. The status meaning is logged and reported to the user if an interactive query. Any additional error information in the Response will be logged.
Failed	Identifier does not match SOP Class	A900	The Association is released and the worklist query is marked as failed. The status meaning is logged and reported to the user if an interactive query. Any additional error information in the Response will be logged.
Failed	Unable to Process	C000 – CFFF	The Association is released and the worklist query is marked as failed. The status meaning is logged and reported to the user if an interactive query. Any additional error information in the Response will be logged.
Pending	Matches are continuing	FF00	The worklist item contained in the Identifier is collected for further processing.
Pending	Matches are continuing Warning that one or more Optional Keys were not supported	FF01	The worklist item contained in the Identifier is collected for later display or further processing. The status meaning is logged only once for each C-FIND operation.
*	*	Any other status	The Association is released and the worklist is marked as failed. The status meaning is logged and reported to the user if an interactive query. Any additional error information in the Response will be logged.



Med X Change, Inc.

## HDMD PRO DICOM Conformance Statement

Document #: 5018-19-F07

Revision: 2.0

Effective Date: Date of last approval

Page: 15 of 26

---

HDMD PRO DICOM Conformance Statement

The behavior of the Workflow AE during communication failure is summarized in the table below.

*Table 4-9 – Modality Worklist Communication Failure Behavior*

Exception	Behavior
Timeout	The Association is aborted using A-ABORT and the worklist query marked as failed. The reason is logged and reported to the user if an interactive query.
Association aborted by the SCP or network layers	The worklist query is marked as failed. The reason is logged and reported to the user if an interactive query.

**4.2.2 Storage AE Specifications**

**4.2.2.1 SOP Classes**

This AE provides standard conformance to the following SOP classes.

*Table 4-10 – SOP classes for Storage AE*

SOP Class Name	SOP Class UID	SCU	SCP
Verification	1.2.840.10008.1.1	Yes	No
SC Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	No
Multi-frame True Color SC mage Storage	1.2.840.10008.5.1.4.1.1.7.4	Yes	No

**4.2.2.2 Association Policies**

**4.2.2.2.1 General**

The DICOM standard application context name for DICOM 3.0 is always proposed.

*Table 4-11 - General DICOM for Worklist AE*

Application Context Name	1.2.840.10008.3.1.1.1
Maximum PDU Size proposed	16384

**4.2.2.2.2 Number of Associations**

*Table 4-12 – Number of Associations as association initiator for Storage AE*

Maximum number of simultaneous associations	1
---	---

**4.2.2.2.3 Asynchronous Nature**

The Storage AE does not support asynchronous communication (multiple outstanding transactions over a single association).



**4.2.2.2.4 Implementation Identifying Information**

*Table 4-13 – DICOM Implementation Class and Version for STORE-SCP*

Implementation Class UID	1.2.276.0.7230010.3.0.9.9.1
Implementation Version Name	MED_X_CHANGE

**4.2.2.3 Association Initiation Policies**

**4.2.2.3.1 Activity – Verify Communications (SCU)**

**4.2.2.3.1.1 Description and Sequencing of Events**

The Storage AE sends DICOM verification requests when the user requests a test of validity of a DICOM connection through the GUI.

**4.2.2.3.1.2 Proposed Presentation Contexts**

The HDMD PRO will propose Presentation Contexts as shown in the following table:

*Table 4-14 – Proposed Presentation Contexts for Activity Verify Communication*

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext Neg.
Name	UID	Name	UID		
Verification	1.2.840.10008	ELE	1.2.840.10008.1.2.1	SCU	None
		ILE	1.2.840.10008.1.2		

**4.2.2.3.1.3 SOP Specific Conformance – Verification SOP Class**

The Storage AE provides standard conformance to the Verification SOP Class as an SCU. If the C-ECHO request was successfully received by external verification SCP, a 0000 (Success) status code will be returned in the C-ECHO response. Otherwise, a C000 (Error – Cannot Understand) status code will be returned in the C-ECHO response.

**4.2.2.3.2 Activity – Send Images**

**4.2.2.3.2.1 Description and Sequencing of Events**

This activity is performed when the device is initiating the image transfer.

The user can select a patient case and request it to be sent to the configured destination. Each request is forwarded to the job queue and processed individually.


The Automatically Upload options allows the user to automatically send a patient case to a pre-configured destination. The option to enable or disable the Automatically Upload feature is configurable by the user from the GUI. When Automatically Upload option is enabled, the captured patient cases get automatically marked for storage. Each marked instance or marked set of instances stored in the database will be forwarded to the network job queue for a pre-configured target destination. The Automatically Upload option is triggered when the user closes the opened patient case. When the Automatically Upload feature is disabled, the user can manually send the patient cases to the destination from the GUI.

## HDMD PRO DICOM Conformance Statement

The Storage AE is invoked by the job control interface that is responsible for processing network storage tasks. The job consists of data describing the instances marked for storage, and the destination to which the instances will be sent. The Storage AE attempts to initiate a new association to issue a C-STORE request. If the Storage AE successfully establishes an association with a remote AE, it will transfer the image corresponding to the marked patient case via the open association. If the patient case consists of multiple images, then each of the images will be transferred over a new association.

If the C-STORE response from the remote application contains a status other than Success or Warning, then the association is released and the related job is switched to a failed state.

The converted DICOM images are converted directly before each association is completed, and are deleted upon closing the association (success or failure).

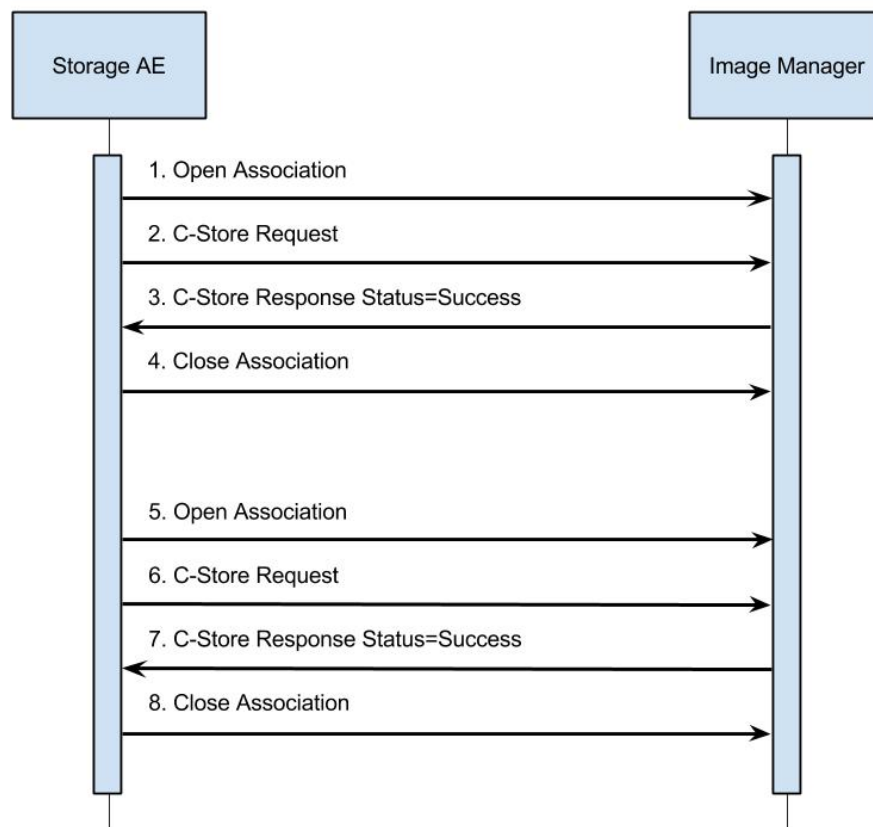

*Figure 4 Sequence of Events – Store Request*

A possible sequence of interactions between the Storage AE and an Image Manager (e.g. a storage device supporting the Storage SOP Class as an SCP) is illustrated in Figure 4.

1. The Storage AE opens an association with the Image Manager.

## HDMD PRO DICOM Conformance Statement

---

2. An acquired image is transmitted to the Image Manager using a C-STORE request.
3. The Image Manager replies with a C-STORE response (status success).
4. The Storage AE closes the association with the Image Manager.
5. The Storage AE opens a new association with the Image Manager.
6. Another acquired image is transmitted to the Image Manager using a C-STORE request.
7. The Image Manager replies with a C-STORE response (status success).
8. The Storage AE closes the association with the Image Manager.

**4.2.2.3.2.2 Proposed Presentation Contexts**

*Table 4-15 – Proposed Presentation Context for Activity Send Images*

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext Neg.
Name	UID	Name	UID		
SC Image Storage	1.2.840.10008.5.1.4.1.1.7	JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50	SCU	None
		JPEG Process 1 Lossy	1.2.840.10008.1.2.4.70	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Implicit VR Endian	1.2.840.10008.1.2	SCU	None
Multi-frame True Color SC Image Storage	1.2.840.10008.5.1.4.1.1.7.4	MPEG4	1.2.840.10008.1.2.4.103	SCU	None

For single frame images, HDMD PRO proposes only JPEG Baseline.

**4.2.2.3.2.3 SOP Specific Conformance for Storage SOP Classes**

The Storage AE maintains a job queue for C-STORE commands. If some of the C-STORE commands in a job fail, then the job will need to be sent manually. Failed or successful jobs will never retry.

*Table 4-16 - C-STORE Response Status Handling Behavior*

Service Status	Further Meaning	Error Code	Behavior
Success	Matching is complete	0000	The SCP has successfully stored the SOP Instance. If all SOP Instances in a send job have status success then the job is marked as completed in the queue and reported to the user via the application.
Refused	Out of Resources	A700-	The Association is released and the send

HDMD PRO DICOM Conformance Statement

		A7FF	job is marked as failed. The status meaning and an error code is logged in the log file and the job failure is reported to the user via the application
Error	Data Set does not match SOP Class	A900-A9FF	The Association is released and the send job is marked as failed. The status meaning and an error code is logged in the log file and the job failure is reported to the user via the application.
Error	Cannot Understand	C000-CFFF	The Association is released and the send job is marked as failed. The status meaning and an error code is logged in the log file and the job failure is reported to the user via the application
Warning	Coercion of Data Elements	B000	Image transmission is considered successful but the status meaning and error code are logged in the log file
Warning	Data Set does not match SOP Class	B007	Image transmission is considered successful but the status meaning and error code are logged in the log file
Warning	Elements Discarded	B006	Image transmission is considered successful but the status meaning and error code are logged in the log file.
*	*	Any other status	The Association is released and the send job is marked as failed. The status meaning and an error code is logged in the log file.

**4.3 Network Interfaces**

HDMD PRO uses TCP/IP as the underlying network implementation.

**4.4 Configuration**

The following items are configurable:

SCU parameters

- Calling AE Title
- Called AE Title
- IP Address
- Port
- Diagnostic logging

Worklist parameters

- Worklist enabled Y/N
- Query
  - Scheduled AE Title

## HDMD PRO DICOM Conformance Statement

- Patient ID
- Modality
- Start date (range)

### Storage parameters

- Storage enabled Y/N
- Automatically Upload
- Upload Videos

### **5 Media Interchange**

HDMD PRO does not support media interchange.

### **6 Support of Character Sets**

HDMD PRO supports ISO-IR 100

### **7 Security**

#### **7.1 Security Profiles**

The HDMD PRO can be configured to use secure DICOM communication in conformance with the Basic TLS Secure Transport Connection Profile

#### **7.2 Application Level Security**

The following security and privacy requirements are defined for HDMD PRO: The GUI contains a login function, including a password, and only authorized users will be able to login to the system.

HDMD PRO DICOM Conformance Statement

**8 Annexures**

**8.1 IOD Contents**

**8.1.1 Secondary Capture IOD**

*Table 8-1 – Secondary Capture IOD*

Module	Attribute	Tag	Value and/or length, range, and origin
PATIENT	Patient Name	(0010,0010)	From MWL or entered by user
	Patient ID	(0010,0020)	From MWL or entered by user
	Patient Sex	(0010,0040)	From MWL or entered by user; M, F, O or empty
	Patient Birth Date	(0010,0030)	From MWL or entered by user
General Study	Study Instance UID	(0020,000D)	From MWL or automatically generated if not present from MWL; not visible on UI
	Study ID	(0020,0010)	Automatically generated; not visible on UI
	Study Date	(0008,0020)	From MWL or automatically created when the study is created
	Study Time	(0008,0030)	From MWL or automatically created when the study is created
	Accession Number	(0008,0050)	From MWL or entered by user
	Referring Physician's Name	(0008,0090)	From MWL or entered by the user
General Series	Modality	(0008,0060)	From MWL or entered by the user
	Series Instance UID	(0020,000E)	Automatically generated
	Series Number	(0020,0011)	1
	Performing Physician Name	(0008,1050)	From MWL or entered by the user
General Image	Instance Number	(0020,0013)	Auto generated
	Patient Orientation	(0020,0020)	Empty, zero length
	Lossy Image Compression	(0028,2110)	01
	Lossy Image Compression Method	(0028,2114)	ISO_10918_1
General Equipment	Conversion Type	(0008,0064)	WSD
	Manufacturer	(0008,0070)	MedXChange
	Station Name	(0008,1010)	From MWL; Not visible on UI
	Manufacturer Model Name	(0008,1090)	HDMD PRO

HDMD PRO DICOM Conformance Statement

	Software Versions	(0018,1020)	The version of the SCU
Image Pixel	Samples per Pixel	(0028,0002)	3
	Photometric Interpretation	(0028,0004)	YBR_FULL_422
	Planar Configuration	(0028,0006)	0
	Rows	(0028,0010)	1080
	Columns	(0028,0011)	1920
	Bits Allocated	(0028,0100)	8
	Bits Stored	(0028,0101)	8
	High Bit	(0028,0102)	7
	Pixel Representation	(0028,0103)	0
	Pixel Data	(7FE0,0010)	From Image
SOP Common Module	SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
	SOP Instance UID	(0008,0018)	Automatically generated
	Character Set	(0008,0005)	ISO_IR 100



HDMD PRO DICOM Conformance Statement

**8.1.2 Multi-frame True Color Secondary Capture IOD**

*Table 8-2 – Multi-frame True Color Secondary Capture IOD*

Module	Attribute	Tag	Value and/or length, range, and origin
PATIENT	Patient Name	(0010,0010)	From MWL or entered by user
	Patient ID	(0010,0020)	From MWL or entered by user
	Patient Sex	(0010,0040)	From MWL or entered by user; M, F, O or empty
	Patient Birth Date	(0010,0030)	From MWL or entered by user
General Study	Study Instance UID	(0020,000D)	From MWL or automatically generated if not present from MWL; not visible on UI
	Study ID	(0020,0010)	Automatically generated; not visible on UI
	Study Date	(0008,0020)	From MWL or automatically created when the study is created
	Study Time	(0008,0030)	From MWL or automatically created when the study is created
	Accession Number	(0008,0050)	From MWL or entered by user
	Referring Physician's Name	(0008,0090)	From MWL or entered by the user
General Series	Modality	(0008,0060)	From MWL or entered by the user
	Series Instance UID	(0020,000E)	Automatically generated
	Series Number	(0020,0011)	1
	Performing Physician Name	(0008,1050)	From MWL or entered by the user
General Image	Instance Number	(0020,0013)	Auto generated
	Patient Orientation	(0020,0020)	Empty, zero length
	Lossy Image Compression	(0028,2110)	01
General Equipment	Manufacturer	(0008,0070)	MedXChange
	Station Name	(0008,1010)	From MWL; Not visible on UI
	Manufacturer Model Name	(0008,1090)	HDMD PRO
	Software Versions	(0018,1020)	The version of the SCU
Image Pixel	Samples per Pixel	(0028,0002)	3
	Photometric Interpretation	(0028,0004)	YBR_PARTIAL_420
	Planar Configuration	(0028,0006)	0
	Rows	(0028,0010)	1080
	Columns	(0028,0011)	1920
	Bits Allocated	(0028,0100)	8

HDMD PRO DICOM Conformance Statement

	Bits Stored	(0028,0101)	8
	High Bit	(0028,0102)	7
	Pixel Representation	(0028,0103)	0
	Pixel Data	(7FE0,0010)	from Video
SOP Common Module	SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7.4
	SOP Instance UID	(0008,0018)	Automatically generated
	Character Set	(0008,0005)	ISO_IR 100

**8.2 Attribute Mapping**

The relationships between attributes received via Modality Worklist and stored in acquired images are summarized in the table below.

*Table 8-3 – Attribute Mapping between Modality Worklist and Image IOD*

Field	MWL Tag	Image Tag	Interface
Patient Name	(0010,0010)	(0010,0010)	Y
Patient ID	(0010,0020)	(0010,0020)	Y
Patient Sex	(0010,0040)	(0010,0040)	Y
Patient Birth Date	(0010,0030)	(0010,0030)	Y
Study Instance UID	(0020,000D)	(0020,000D)	N
Study Date	(0040,0002)	(0008,0020)	Y
Study Time	(0040,0003)	(0008,0030)	Y
Accession Number	(0008,0050)	(0008,0050)	Y
Referring Physician's Name	(0008,0090)	(0008,0090)	Y
Modality	(0008,0060)	(0008,0060)	Y
Performing Physician Name	(0040,0006)	(0008,1050)	Y
Station Name	(0040,0010)	(0008,1010)	N